

Prepared for:

Centers for Medicare & Medicaid Services and The Office of
the National Coordinator for Health Information Technology

CMS Alliance to Modernize Healthcare
Federally Funded Research and Development Center



An Open Source Electronic Clinical Quality Measure Testing and
Certification Tool

Cypress User Guide

Version 4.0

July 27, 2018

The views, opinions, and/or findings contained in this report are those of The MITRE Corporation and should not be construed as official government position, policy, or decision unless so designated by other documentation.

This document was prepared for authorized distribution only. It has not been approved for public release.

© 2017, The MITRE Corporation. All Rights Reserved.

Record of Changes

Version	Date	Author / Owner	Description of Change
3.0	August 15, 2016	ONC/CAMH	Version 3.0 for release
3.2	July 27, 2017	CAMH	Version 3.2 for release
4.0	July 27, 2018	CAMH	Version 4.0 for release

About the CMS Alliance to Modernize Healthcare

The Centers for Medicare & Medicaid Services (CMS) sponsors the CMS Alliance to Modernize Healthcare (CAMH), the first Federally Funded Research and Development Center (FFRDC) dedicated to strengthening our nation's healthcare system.

The CAMH FFRDC enables CMS, the Department of Health and Human Services (HHS), and other government entities to access unbiased research, advice, guidance, and analysis to solve complex business, policy, technology, and operational challenges in health mission areas. The FFRDC objectively analyzes long-term health system problems, addresses complex technical questions, and generates creative and cost-effective solutions in strategic areas such as quality of care, new payment models, and business transformation.

Formally established under Federal Acquisition Regulation (FAR) Part 35.017, FFRDCs meet special, long-term research and development needs integral to the mission of the sponsoring agency—work that existing in-house or commercial contractor resources cannot fulfill as effectively. FFRDCs operate in the public interest, free from conflicts of interest, and are managed and/or administered by not-for-profit organizations, universities, or industrial firms as separate operating units.

The CAMH FFRDC applies a combination of large-scale enterprise systems engineering and specialized health subject matter expertise to achieve the strategic objectives of CMS, HHS, and other government organizations charged with health-related missions. As a trusted, not-for-profit adviser, the CAMH FFRDC has access, beyond what is allowed in normal contractual relationships, to government and supplier data, including sensitive and proprietary data, and to employees and government facilities and equipment that support health missions.

CMS conducted a competitive acquisition in 2012 and awarded the CAMH FFRDC contract to The MITRE Corporation (MITRE). MITRE operates the CAMH FFRDC in partnership with CMS and HHS, and maintains a collaborative alliance of partners from nonprofits, academia, and industry. This alliance provides specialized expertise, health capabilities, and innovative solutions to transform delivery of the nation's healthcare services. Government organizations and other entities have ready access to this network of partners, including RAND Health, the Brookings Institution, and other leading healthcare organizations. This includes select qualified small and disadvantaged business.

The FFRDC is open to all CMS and HHS Operating Divisions and Staff Divisions. In addition, government entities outside of CMS and HHS can use the FFRDC with permission of CMS, CAMH's primary sponsor.

Table of Contents

1. Introduction	1
2. Cypress Testing Capabilities	2
2.1 Capture/Record and Export.....	2
2.2 Import and Calculate	3
2.3 Electronic Submission.....	4
2.4 Data Filtering.....	5
3. Detailed Description of Cypress Workflow	6
3.1 Accessing Cypress.....	7
3.2 Overview of Administrative Functions	8
3.2.1 Master Patient List	9
3.2.2 Account.....	11
3.2.3 Log Out	12
3.2.4 Add Vendor.....	12
3.2.5 Edit Vendor.....	13
3.3 Cypress v4.0 Preparation for Testing	14
3.4 Test Execution.....	20
3.4.1 Automated Measure Test Execution.....	21
3.4.2 Record Sample Test	26
3.4.3 CQM Filtering Test.....	29
3.5 Test Execution Success Criteria.....	30
3.6 Submit	32
3.7 Verify	33
Acronyms	34

List of Figures

Figure 1. Capture/Record and Export	3
Figure 2. Import, Calculate, and Electronic Submission	5
Figure 3. Cypress Workflow in an Authorized Testing Lab.....	6
Figure 4. Cypress Sign In Page.....	7
Figure 5. Cypress Terms and Conditions Page	8
Figure 6. Cypress Account Creation	8
Figure 7. Cypress Dashboard	9
Figure 8. Master Patient List of Test Patients	9
Figure 9. Patients Specific to CMS2v5 Preventive Care and Screening: Screening for Clinical Depression and Follow-Up Plan Patients	10
Figure 10. Patient Test Record Data Requirements and eCQM Qualifiers	11
Figure 11. Account Password Update	12
Figure 12. Cypress v4.0 Log Out.....	12
Figure 13. Add Vendor Page.....	13
Figure 14. Edit Vendor Page.....	13
Figure 15. Dashboard Select Add Vendor.....	14
Figure 16. Create Vendor Page.....	15
Figure 17. Dashboard with New Vendor Created.....	15
Figure 18. Vendor Product Information Page.....	16
Figure 19. Vendor Add Product Page	17
Figure 20. Eligible Hospital eCQMs Measure Selection.....	18
Figure 21. Vendor Add Product, “Custom” Measures Option	18
Figure 22. Vendor Add Product page, Select “Add Product”.....	19
Figure 23. Dashboard Displaying a Vendor with Two Products Added	20
Figure 24. C1-C2 Automated Entry Certification.....	21
Figure 25. Add Product for Automated Entry of Measure Data.....	22
Figure 26. Selecting A Product to Test.....	22
Figure 27. Showing C1 Record Sample, C1 Automated, and C2 Product Measures	23
Figure 28. Product Measure Upload or Measure Name Selection.....	23
Figure 29. Individual Measure Test Page	24
Figure 30. Zip File of Patient Test Data for Selected eCQM	24

Figure 31. Listing of Zip File of XML Patient Test Data for Testing Selected eCQM..... 25

Figure 32. Patient XML File for C2 Test..... 25

Figure 33. Upload Test Execution Results 26

Figure 34. Example of Test Execution Summary Results 26

Figure 35. Record Sample Test, Select "View Test" 27

Figure 36. Record Sample Page..... 27

Figure 37. View listing of valid codes 28

Figure 38. Search for valid codes 28

Figure 39. Complete and Save a Test 29

Figure 40. Select File to Upload 29

Figure 41. Select a Category I or Category III to Test..... 30

Figure 42. Category I Test Page for Median Time from ED Arrival to ED Departure for Discharged ED Patients 30

Figure 43. Measure Test Failure Messages..... 32

1. Introduction

Cypress v4.0 is the rigorous and repeatable testing tool of Electronic Health Records (EHR) and health information technology (IT) modules used in calculating electronic Clinical Quality Measures (eCQM). Cypress v4.0 is the official testing tool for the 2015 EHR Certification program supported by the Office of the National Coordinator for Health Information Technology (ONC). The 2015 Edition final rule, published by the ONC, updates the ONC Health IT Certification Program and includes certification criteria to support electronic clinical quality measurement (eCQM) and reporting across the healthcare ecosystem. The 2015 Edition eCQM certification criteria also support the requirements of the Centers for Medicare & Medicaid Services (CMS) Promoting Interoperability Program and other CMS program requirements.

ONC and CMS developed the Cypress v4.0 User Guide for test proctors who test and certify EHRs and health IT modules at Authorized Testing Labs (ATL). EHR software engineers, quality assurance engineers, and production release engineers may draw on the guide when they use Cypress in a pre-testing mode to understand how their health IT product will perform in an ATL-conducted operational test.

This guide provides instructions on how to use the open source Cypress v4.0 tool (it is assumed the user has downloaded the software). It addresses the requirements and steps for testing health IT products for calculating and reporting eCQMs.

The Cypress tool is freely available for use or adoption by the health IT community, including EHR vendors and testing labs. The open source project website at [Project Cypress](#) provides information detailing the set up and configuration of Cypress v4.0 open source software.

2. Cypress Testing Capabilities

To achieve certification pursuant to the most recent 2015 standards, each health IT product must show that it meets four criteria by demonstrating required capabilities specified in the regulation and described in the following subsections. The Cypress v4.0 software verifies four required eCQM capabilities for health IT certification (Capture/Record and Export, Import and Calculate, Electronic Submission, and Data Filtering), as described in the following sections.

2.1 Capture/Record and Export

Cypress v4.0 supports the requirements for Capture/Record and Export capabilities as follows:

- **Capture/Record** – To be certified in accordance with 45 CFR §170.315(c), the technology must be able to electronically capture/record all of the data identified in the specified procedure necessary to calculate each eCQM. Data required for eCQM exclusions or exceptions must be codified entries. These entries may include specific terms as defined by each eCQM, or may include codified expressions, such as “patient reason,” “system reason,” or “medical reason.”
- **Export** – As provided in 45 CFR §170.315(c)(1), the technology must be able to electronically export a data file formatted in accordance with the Quality Reporting Document Architecture (QRDA) Category I standard that includes all of the data captured for each and every eCQM for which the technology is being certified.

The functionality requirement for Capture/Record and Export specifies that a system user can record and export individual, patient-level eCQM data formatted to the Health Level Seven International (HL7) QRDA Category I Release 5 Implementation Guide (IG) at any time the user chooses, for one or multiple patients, without needing developer support. The requirement for Capture/Export is part of the certification criteria necessary to satisfy the 2015 Edition Base EHR definition. The capability to export eCQM data serves two purposes: (1) a provider or health system can view and verify their eCQM results for quality improvement on a near real-time basis, and (2) providers can export their results to multiple programs, such as those run by CMS, states, and private payers.

Figure 1 depicts the basic concept for Capture/Record and Export. The primary purpose of this step is to verify the technology’s ability to export data in the proper QRDA Category I format with the proper Quality Data Model (QDM) data elements.

To verify this capability, Cypress produces static patient data for each of the eCQMs that are to be tested, and exports the relevant patients. This data is entered into the technology. The technology is then commanded to export the patient test data as a set of QRDA Category I files that contain the proper elements from the QDM for calculating the eCQMs under test. These QRDA files are loaded back into Cypress where they are tested for validity, determining valid QRDA Category I Extensible Markup Language (XML) documents, and correctness, containing only the elements required to calculate the eCQMs.

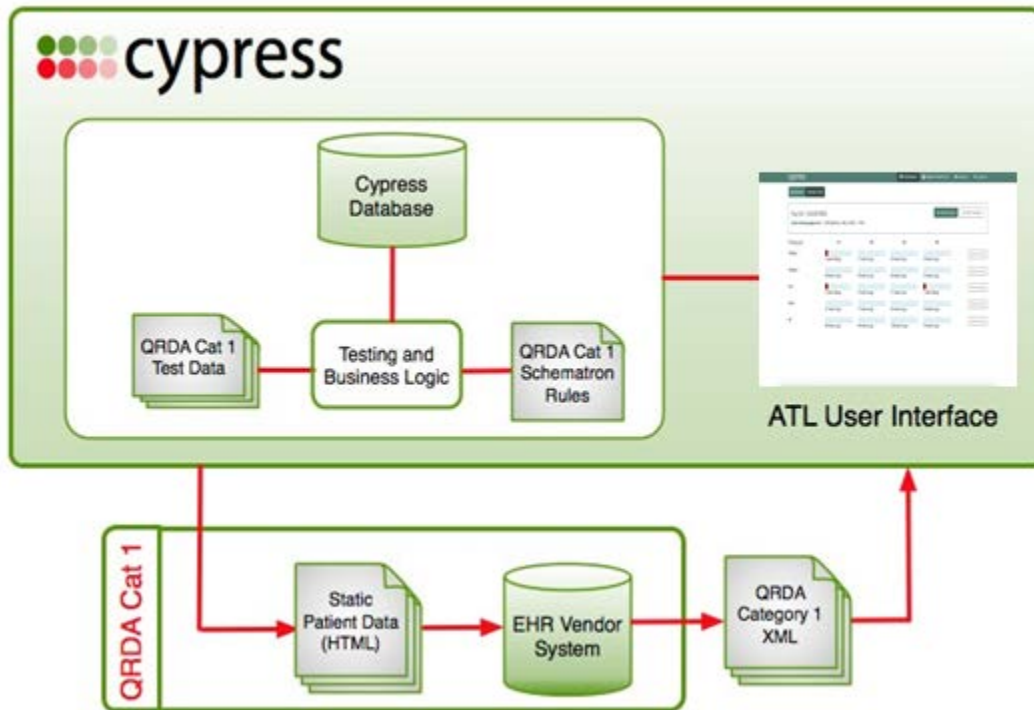


Figure 1. Capture/Record and Export

2.2 Import and Calculate

Cypress v4.0 supports the requirements for Import and Calculate capabilities as follows:

- **Import** – The technology must be able to electronically import a data file formatted in the QRDA Category I format.
- **Calculate** – The technology must be able to electronically calculate each and every clinical quality measure for which it is presented for certification.

A Health IT Module must be capable of demonstrating that it can import data to warrant certification against this criterion using the QRDA Category I IG, even if the module is also certified to provide “capture/record and export” and “report” functions.¹ The requirement ensures that users of certified health IT can import eCQM data formatted to the QRDA Category I standard for one or more patients without needing to request developer support.

¹ From Federal Regulation (80 FR 62650-62651): “First, this functionality could streamline the testing and certification process by importing QRDA Category I files rather than systems needing to manually enter test patient data. Second, the import functionality can promote quality improvement and data sharing between systems by providing systems the ability to import CQM data from other systems in a standardized format.”

2.3 Electronic Submission

Cypress v4.0 supports the requirements for Electronic Submission capabilities as follows:

- Electronic Submission enables a user to electronically create a data file in QRDA Category III format for transmission of clinical quality measurement data that can be electronically accepted by CMS.

The criterion for certification of Electronic Submission capabilities supports eCQM reporting using the consensus, industry-based QRDA Category I Release 5 and QRDA Category III Release 2.1 IGs. It also supports better alignment with the reporting requirements of CMS programs. The CMS reporting requirements (e.g., use of the CMS QRDA IG) are included as an optional provision within the criterion because not all certified health IT is intended for CMS reporting. The certification to the HL7 QRDA Category I and III standards provide a baseline for interoperability of eCQM data because these standards are consensus based and industry developed. Moreover, the program-agnostic HL7 QRDA standards can support several use cases for exchanging eCQM data.

Figure 2 shows the basic concept for Import, Calculate, and Electronic Submission. These steps provide for automated verification that a health IT product can:

- Import and calculate the eCQM results for the quality measures being certified based on the synthetic patient data that Cypress presents to the technology under test
- Generate a properly formatted summary eCQM report that could be electronically submitted using QRDA Category III format

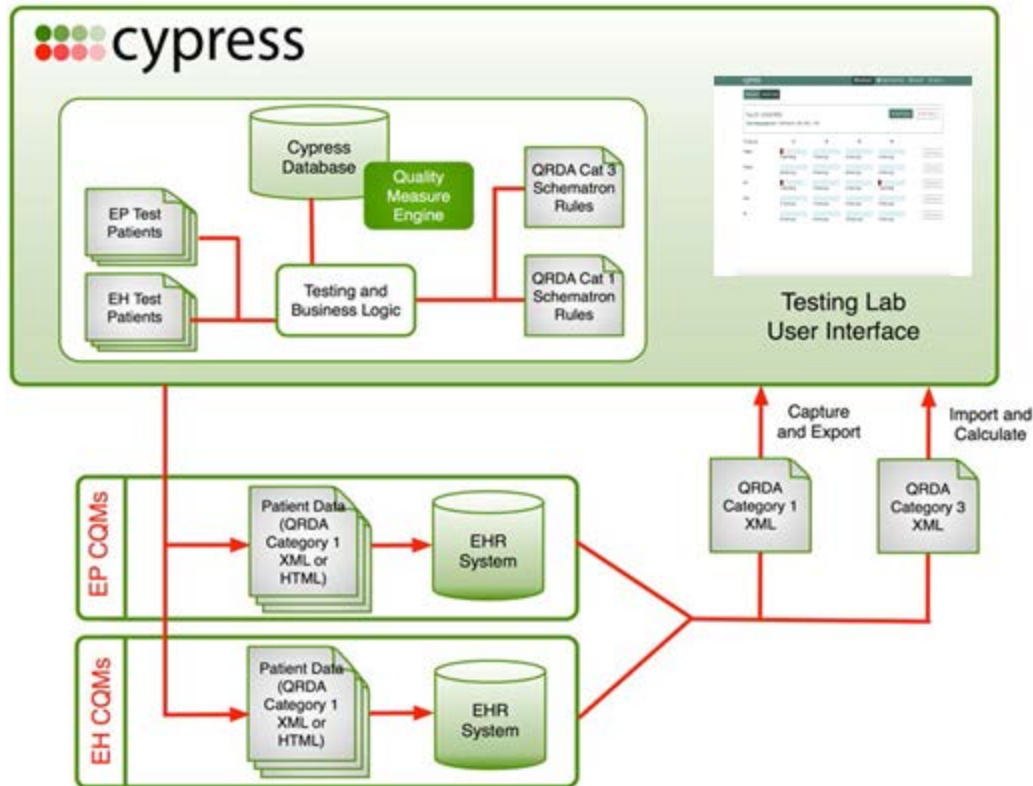


Figure 2. Import, Calculate, and Electronic Submission

2.4 Data Filtering

Cypress v4.0 supports the requirements for Data Filtering capabilities as follows:

- The technology must be able to record data (according to specified standards, where applicable) and filter eCQM results at both patient and aggregate levels.²

Filtering individual patient-level and aggregate-level eCQM results by data supports administrative reporting as well as identification of health disparities and gaps in care for patients treated at particular group practice sites or in a given Accountable Care Organization (ACO).

² Rule Reference: 2015 Edition Health Information Technology (Health IT) Certification Criteria, Base Electronic Health Record (EHR) Definition, and ONC Health IT Certification Program Modifications Final Rule (The “2015 Edition”): “The filter functionality included in this criterion will allow a provider to make a query for eCQM results using one or a combination of data captured by the certified health IT for quality improvement and quality reporting purposes. It can also aid in the identification of health disparities, enable care quality improvement, and support providers in delivering more effective care to their patient populations. These filters include, but are not limited to, practice site address, patient age, patient sex, and patient problem list.”

3. Detailed Description of Cypress Workflow

Figure 3 illustrates the general workflow of a test performed with the Cypress open source software tool and a description of how the test procedure is organized and conducted. The augmentation of the test procedure to include Cypress is based on the ONC-approved and the National Institute of Standards and Technology (NIST)-published procedure for testing the accurate calculation, submission, and degree of correctness of eCQMs.

As shown in Figure 3, the vendor interacts with the vendor system. An ATL test proctor interacts with the Cypress web interface. The test proctor downloads test data from Cypress, which is then sent from Cypress and entered into the vendor system. The vendor returns test results to Cypress, which generates reports reflecting assessment of certification testing.

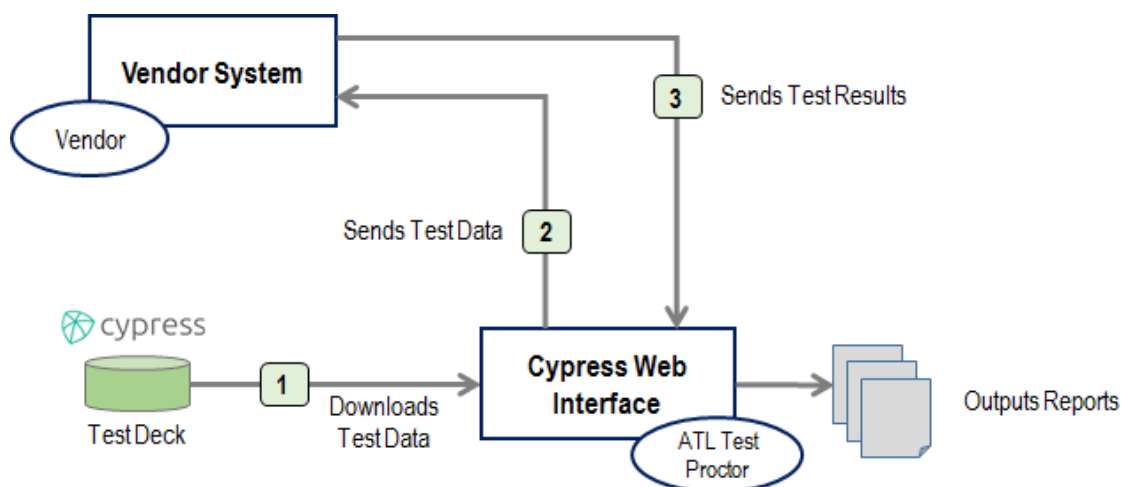


Figure 3. Cypress Workflow in an Authorized Testing Lab

Cypress can perform the following types of tests in support of eCQM certification:

1. XML Data conformance testing of the QRDA Category I standard for individual patient-level data used for eCQM calculation
2. XML Data conformance testing of the QRDA Category III standard for aggregate reporting of eCQM calculation
3. Accuracy calculation testing of the Eligible Professional / Eligible Clinician eCQMs
4. Accuracy calculation testing of the Eligible Hospital / Critical Access Hospital eCQMs

The Cypress website provides a complete description of the Cypress Testing Procedure (available at <http://healthit.gov/cypress/resources.html>).

The following subsections present a detailed description of Cypress v4.0, from accessing Cypress, overview of administrative functions, preparation for testing, test execution, exit success criteria, and submission to verification.

3.1 Accessing Cypress

To access and download the Cypress Software, go to [Project Cypress](#):

- The Project Cypress site provides several options and detailed instructions for downloading and installing the Cypress software. If the software has not been installed, please follow the Cypress Download Instructions located on the Project Cypress site. This User Guide does not provide instructions for downloading the Cypress software.

After Cypress is downloaded and installed, it is accessible via a URL, bookmark, or icon you created as part of the download/installation process.

Upon accessing the installed instance of Cypress, the Sign In screen should appear. Figure 4 presents a screenshot of the “Sign In” screen. To create an account, select **Sign Up**.

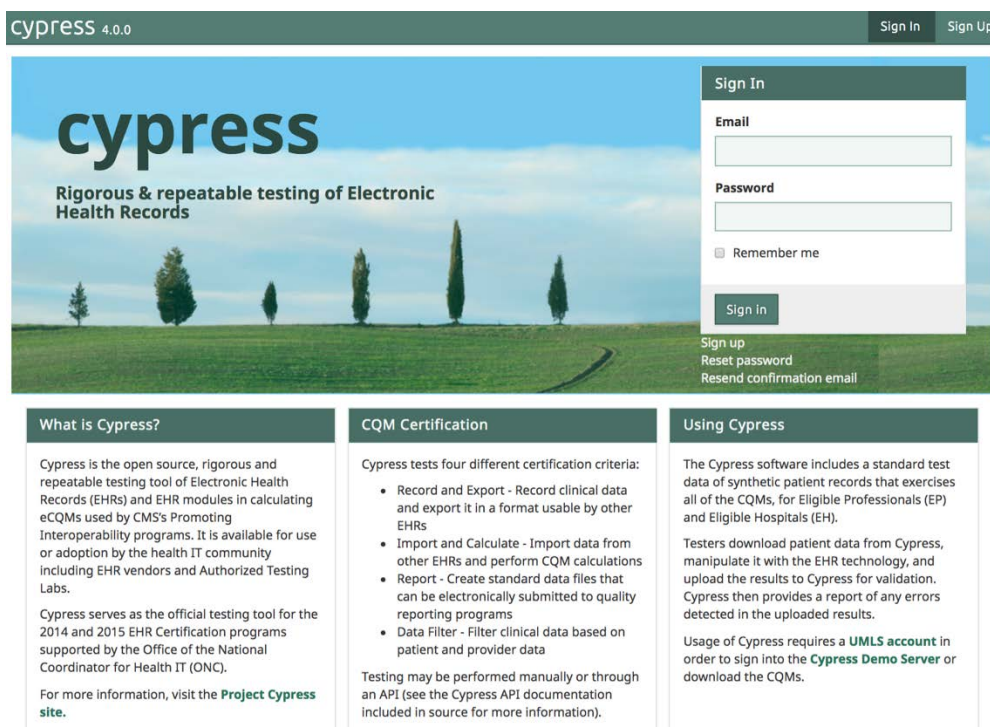


Figure 4. Cypress Sign In Page

- If you have previously set up an account, enter your email and password, and select **Sign In**.
- If you have previously created an account and forgotten your password, select **Reset password**. In the **Forgot your Password?** screen, enter the email address associated with your Cypress account, and select **Send me reset password instructions**. You will be sent a link to reset your password.
- **Sign Up** will bring you to the Sign Up and Terms and Conditions page. Click on the **Terms and Conditions** link on that page. Figure 5 presents a screenshot of the Terms and Conditions page.

Terms and Conditions for use of Cypress

Performance measures and related data specifications (the "Measures") are copyrighted by the noted quality measure providers as indicated in the applicable Measure. Coding vocabularies are owned by their copyright owners. By using the Measures, a user ("User") agrees to these Terms of Use. Measures are not clinical guidelines and do not establish a standard of medical care and quality measure providers are not responsible for any use of or reliance on the Measures.

THE MEASURES AND SPECIFICATIONS ARE PROVIDED "AS IS" WITHOUT ANY WARRANTY OF ANY KIND, AND ANY AND ALL IMPLIED WARRANTIES ARE HEREBY DISCLAIMED, INCLUDING ANY WARRANTY OF NON-INFRINGEMENT, ACCURACY, MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. NO QUALITY MEASURE PROVIDER, NOR ANY OF THEIR TRUSTEES, DIRECTORS, MEMBERS, AFFILIATES, OFFICERS, EMPLOYEES, SUCCESSORS AND/OR ASSIGNS WILL BE LIABLE TO YOU FOR ANY DIRECT, INDIRECT, SPECIAL, EXEMPLARY, INCIDENTAL, PUNITIVE, AND/OR CONSEQUENTIAL DAMAGE OF ANY KIND, IN CONTRACT, TORT OR OTHERWISE, IN CONNECTION WITH THE USE OF THE CYPRESS TOOL OR THE MEASURES, EVEN IF ADVISED OF THE POSSIBILITY OF SUCH LOSS OR DAMAGE.

The Measures are licensed to a User for the limited purpose of using, reproducing and distributing the Measures with the Cypress Tool as delivered to User, without any modification, for commercial and noncommercial uses, but such uses are only permitted if the copies of the Measures contain this complete Copyright, Disclaimer and Terms of Use. Users of the Measures may not alter, enhance, or otherwise modify the Measures.

NOT A CONTRIBUTION - The Measures, including specifications and coding, as used in the Cypress Tool, are not a contribution under the Apache license. Coding in the Measures is provided for convenience only and necessary licenses for use should be obtained from the copyright owners. Current Procedural Terminology (CPT®) © 2004-2010 American Medical Association. LOINC® © 2004 Regenstrief Institute, Inc. SNOMED Clinical Terms® (SNOMED CT®) © 2004-2010 International Health Terminology Standards Development Organization.

[Back](#)

Figure 5. Cypress Terms and Conditions Page

- To **Sign up**, enter your Email, a Password, and then confirm that Password.
- Read the Terms and Conditions, check **I agree to the above Terms and Conditions**, and select **Sign up** to create your Cypress Account as shown in the screenshot of the Cypress Account creation page (Figure 6).

Sign Up

Email

Password

8 characters minimum and include at least 3 of the following: lowercase letters, uppercase letters, digits, and special characters.

Confirm Password

Terms and Conditions

I agree to the above Terms and Conditions

Sign up

[Sign in](#)
[Resend confirmation email](#)

Figure 6. Cypress Account Creation

3.2 Overview of Administrative Functions

Cypress displays the **Dashboard** after you create your account, as shown in Figure 7.



Figure 7. Cypress Dashboard

The Dashboard includes the following Cypress Administrative Functions:

1. Master Patient List – Provides a list of all test data for eCQMs
2. Account – Update a Cypress Account Password
3. Log Out – Log out of the Cypress Application
4. Add Vendor – Add vendor by entering EHR Vendor contact and product information (please refer to “Cypress v4.0 Preparation for Testing”, subsection 4.3)
5. Edit EHR Vendor – Edit EHR Vendor contact and product information (please refer to “Cypress v4.0 Preparation for Testing”, subsection 4.3)

3.2.1 Master Patient List

Figure 8 presents the Master Patient List page that provides a list of all test data for eCQMs for calendar year 2019 reporting.

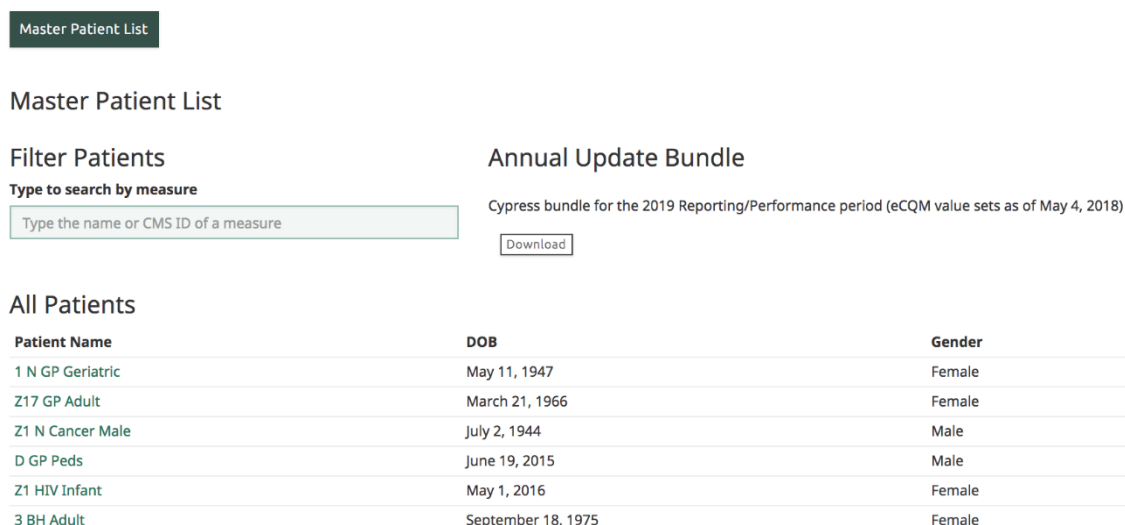


Figure 8. Master Patient List of Test Patients

By selecting the **Filter by Measure** drop-down, you can select a specific measure from a list of patient records that apply to a specific eCQM and eCQM qualifiers. Figure 9 presents an example screenshot of filtering by the measure, CMS2v8 Preventive Care and Screening: Screening for Clinical Depression and Follow-Up Plan Patients.

Master Patient List

Master Patient List

Filter Patients

Type to search by measure

cms2

Annual Update Bundle

Cypress bundle for the 2019 Reporting/Performance period (eCQM value sets as of May 4, 2018)

Download

CMS2v8 Preventive Care and Screening: Screening for Depression and Follow-Up Plan Patients

Patient Name	DOB	Gender	IPOP	DENOM	DENEX	NUMER	DENEXCEP
1 N GP Geriatric	May 11, 1947	Female	●	●	○	○	○
Z17 GP Adult	March 21, 1966	Female	●	●	○	○	○
Z1 N Cancer Male	July 2, 1944	Male	●	●	○	○	○
3 BH Adult	September 18, 1975	Female	●	●	●	○	○
Z13 N GP Adult	February 13, 1969	Male	●	●	○	○	○
B HIV Peds	November 1, 2002	Female	●	●	○	○	●
Z11 Heart Adult	March 12, 1959	Female	●	●	○	○	○
Z15 N GP Adult	February 15, 1969	Male	●	●	○	○	○

Figure 9. Patients Specific to CMS2v5 Preventive Care and Screening: Screening for Clinical Depression and Follow-Up Plan Patients

If you click on the patient's name in the patient record list, Cypress will display an individual patient record and their eCQM qualifiers as shown in Figure 10.


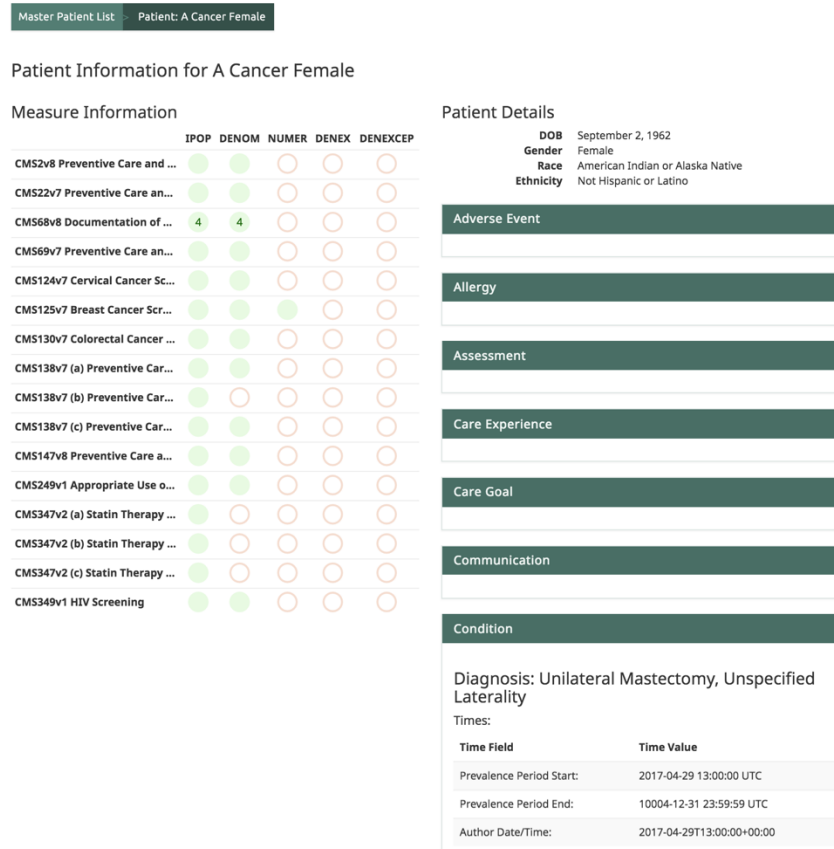


Figure 10. Patient Test Record Data Requirements and eCQM Qualifiers

3.2.2 Account

If you have previously set up an account, this function allows you to change your Password or delete your account. Figure 11 presents a screenshot of the account password update and delete page.

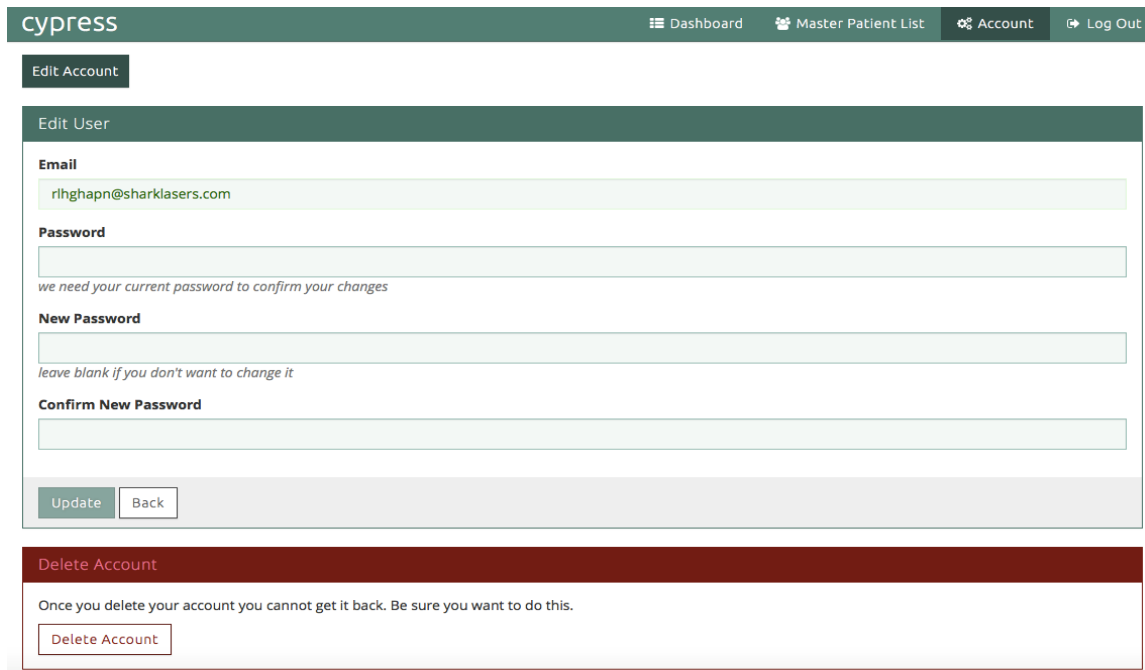

The screenshot shows the 'Edit User' form in the Cypress application. The form is titled 'Edit User' and contains the following fields and controls:

- Email:** A text input field containing the email address 'rlhghapn@sharklasers.com'.
- Password:** A text input field for the current password. Below it, a note reads: 'we need your current password to confirm your changes'.
- New Password:** A text input field for the new password. Below it, a note reads: 'leave blank if you don't want to change it'.
- Confirm New Password:** A text input field for confirming the new password.
- Buttons:** At the bottom of the form, there are two buttons: 'Update' and 'Back'.

Below the 'Edit User' form, there is a section titled 'Delete Account' with a warning message: 'Once you delete your account you cannot get it back. Be sure you want to do this.' and a 'Delete Account' button.

Figure 11. Account Password Update

3.2.3 Log Out

Figure 12 presents a screenshot of the Log Out function that allows a user to return to the Account Sign in (as shown in Figure 4).

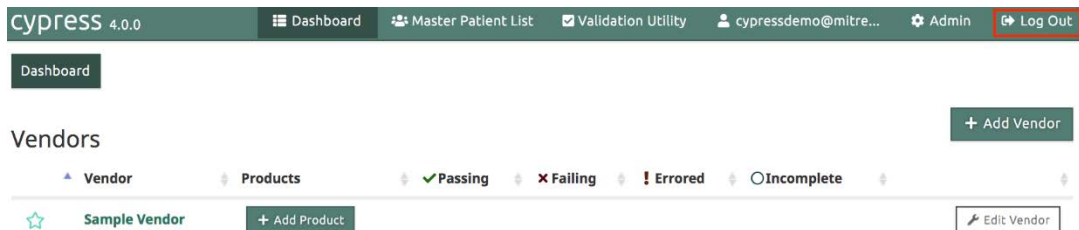


Figure 12. Cypress v4.0 Log Out

3.2.4 Add Vendor

The Add Vendor function allows the user to enter EHR vendor contact and product information (as described in subsection 3.3, Cypress v4.0 Preparation for Testing) as shown in Figure 13.

Dashboard > Add Vendor

Add Vendor

Vendor Name

Vendor ID

URL

Address

State

Zip

Add Point of Contact

Add Vendor Cancel

Figure 13. Add Vendor Page

3.2.5 Edit Vendor

The Edit Vendor function allows a user to edit EHR Vendor contact and product information (as described in subsection 3.3, Cypress v4.0 Preparation for Testing) as shown in Figure 14.

Dashboard > Vendor: Sample Vendor > Edit Vendor

Save Changes: Sample Vendor

Vendor Name
Sample Vendor

Vendor ID
ID 1

URL
www.samplevendor.com

Address
1287 enterprise way

State
DC

Zip
20013

POC Name
John Doe

Email
johndoe@samplevendor.com

Telephone
111-111-1111

Type of Contact
Manager

Remove

Add Point of Contact

Save Changes Cancel

Delete Vendor

Removing a vendor will also delete all associated products, product tests, and test execution results. Be sure you want to do this.

Delete Vendor

Figure 14. Edit Vendor Page

3.3 Cypress v4.0 Preparation for Testing

Add Vendor Information

- Once you have created an account, you can begin testing by adding a Vendor and Contact Information.
- Select **Add Vendor** from the Dashboard as shown in Figure 15.

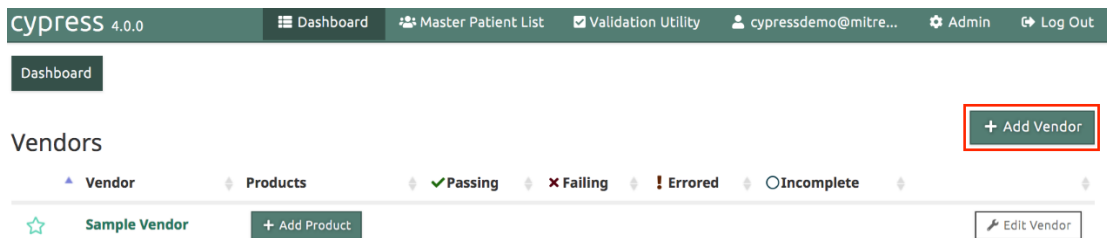


Figure 15. Dashboard Select Add Vendor

- After selecting **Add Vendor**, the **Create Vendor** information will be displayed as shown in Figure 16.
- Complete the fields listed under Create Vendor and select **Create Vendor**.

Dashboard > Add Vendor

Add Vendor

Vendor Name
Sample Vendor

Vendor ID
ID 2

URL
www.samplevendor.com

Address
1287 enterprise way

State
DC

Zip
20013

POC Name **Email** **Telephone** **Type of Contact** **Remove**

John Doe johndoe@samplevendor.com 111-111-1111 Manager

Add Point of Contact

Add Vendor Cancel

Figure 16. Create Vendor Page

Enter Product Information

- The next step is to enter Product Information. Begin by clicking the Vendor name displayed on the Dashboard as shown in Figure 17.

Dashboard

Vendors + Add Vendor

Vendor Products ✓ Passing ✗ Failing ! Errored ○ Incomplete

☆ **Sample Vendor** + Add Product Edit Vendor

Figure 17. Dashboard with New Vendor Created

- Next, click **Add Product**, as shown in Figure 18, to begin entering vendor product information.

The screenshot shows a web interface for a vendor. At the top, there are two tabs: 'Dashboard' and 'Vendor: Sample Vendor'. Below the tabs, the main content area displays the vendor's information: 'Sample Vendor (ID: ID 1)' with an 'Edit Vendor' button. The vendor details include a website URL (http://www.samplevendor.com), address (1287 enterprise way, DC, 20113), manager name (John Doe), email (johndoe@samplevendor.com), and phone number ((111) 111-1111). Below the vendor information, there is a section titled 'Start EHR Certification with' and a button labeled '+ Add Product' which is highlighted with a red border.

Figure 18. Vendor Product Information Page

- On the **Vendor Add Product** page, presented in Figure 19:
 - Enter Product information (Name, Version, and Description). Examples would be: product version number, the name and version of any optional modules installed in the product at the time of the test, and the operating system.
 - For Certification Types, a product must, at a minimum, certify to either the C1 test or the C2 test. To indicate which tests are being certified, check the box selecting from the following options:
 - ◆ C1 Test – Record and Export
 - ◆ C2 Test – Import and Calculate
 - ◆ C3 Test – Data Submission
 - ◆ C4 Test – Data Filtering
 - For Records Options, note that Randomize Records and Duplicate Records have already been pre-checked because these options are recommended for the most robust testing (although they can be unselected, if needed)
 - For Annual Update Bundle, you must select which bundle of eCQMs you are certifying for:
 - ◆ Cypress bundle for the 2019 Reporting/Performance period (eCQM value sets as of May 4, 2018)

Dashboard > Vendor: Sample Vendor > Add Product

Add Product

Name

Version

Description

Certification Types

C1 Test

C2 Test

C3 Test

C4 Test

Select the certification type Cypress should use to certify this product

Records Options

Randomize Records

Duplicate Records

Recommended for most robust testing.

Annual Update Bundle

Cypress bundle for the 2019 Reporting/Performance period (eCQM value sets as of May 4, 2018)

Shift Records

Selecting Shift Records will move patient data forward into the appropriate reporting period. Otherwise patient data will remain in a previously completed calendar year.

Measures Options

Eligible Hospital eQMs

Eligible Professional eQMs

All eQMs

Custom...

Indicate the clinical quality measures Cypress should use to certify this product. Testing will be performed on a measure-by-measure basis. Click 'Custom' to specify individual measures.

Figure 19. Vendor Add Product Page

- The Vendor Add Product page also has a section entitled “Measures Options” that must be completed before adding a product. For Measures Options, you must indicate the clinical quality measures (i.e., select one option) Cypress should use to certify this product, as shown in Figure 20. The options are:
 - Eligible Hospital eQMs
 - Eligible Provider eQMs
 - All eQMs
 - Custom. Selecting “Custom” allows you to specify any individual measures Cypress should use to certify this product. Figure 21 presents a screenshot of the option for “Custom”.

Dashboard Vendor: Sample Vendor > Add Product

Add Product

Name

Version

Description

Certification Types

- C1 Test
- C2 Test
- C3 Test
- C4 Test

Select the certification type Cypress should use to certify this product

Records Options

- Randomize Records
- Duplicate Records

Recommended for most robust testing.

Annual Update Bundle
 Cypress bundle for the 2019 Reporting/Performance period (eCQM value sets as of May 4, 2018)

- Shift Records

Selecting Shift Records will move patient data forward into the appropriate reporting period. Otherwise patient data will remain in a previously completed calendar year.

Measures Options

- Eligible Hospital eCQMs
- Eligible Professional eCQMs
- All eCQMs
- Custom...

Indicate the clinical quality measures Cypress should use to certify this product. Testing will be performed on a measure-by-measure basis. Click 'Custom' to specify individual measures.

Figure 20. Eligible Hospital eCQMs Measure Selection

Dashboard Vendor: Sample Vendor > Add Product

Add Product

Name

Version

Description

Certification Types

- C1 Test
- C2 Test
- C3 Test
- C4 Test

Select the certification type Cypress should use to certify this product

Records Options

- Randomize Records
- Duplicate Records

Recommended for most robust testing.

Annual Update Bundle
 Cypress bundle for the 2019 Reporting/Performance period (eCQM value sets as of May 4, 2018)

- Shift Records

Selecting Shift Records will move patient data forward into the appropriate reporting period. Otherwise patient data will remain in a previously completed calendar year.

Measures Options

- Eligible Hospital eCQMs
- Eligible Professional eCQMs
- All eCQMs
- Custom...

Indicate the clinical quality measures Cypress should use to certify this product. Testing will be performed on a measure-by-measure basis. Click 'Custom' to specify individual measures.

Figure 21. Vendor Add Product, "Custom" Measures Option

- Please note that testing will be performed on a measure-by-measure basis.
- Once all of the information has been entered on the Vendor Add Product page, select **Add Product**, as shown in Figure 22.

The screenshot shows a web interface for selecting custom measures. At the top, there is a header "Select Custom Measures 16" with a dropdown arrow and a "Clear all" button. Below this is a search bar labeled "Type to filter by measure" with the placeholder text "Type a keyword or CMS ID of a measure". A table lists various measures with checkboxes and counts. The measure "CMS53v7 Primary PCI Received Within 90 Minutes of Hospital Arrival (EH)" is selected. At the bottom, there are two buttons: "Add Product" (highlighted with a red box) and "Cancel".

Measure Name	Count	Selected
Acute Myocardial Infarction (1 EH)	1	✓
Asthma (1 EH)	1	✓
Behavioral Health Adult (7 EP)		
Behavioral Health General (1 EP)		
Behavioral Health Pediatric (1 EP)		
Cancer (2 EP)		
Community/Population Health (1 EP)		
Core (15 EP)		
Dental (1 EP)		
Diabetes (5 EP)		
Effective Clinical Care (2 EP)		
Efficiency and Cost Reduction (1 EP)		
Emergency Department (3 EH)	3	✓
Eye (4 EP)		
General Practice Adult (7 EP)		
General Practice Pediatric (1 EP)		
HIV (1 EP)		
Heart (4 EP)		
Newborn (2 EH)	2	✓
Orthopedics (2 EP)		
Pregnancy (1 EP, 1 EH)	1	✓
Stroke (6 EH)	6	✓
Venous Thromboembolism (2 EH)	2	✓
CMS53v7 Primary PCI Received Within 90 Minutes of Hospital Arrival (EH)		✓

Figure 22. Vendor Add Product page, Select "Add Product"

- The Vendor and Product will now display on the Dashboard.
- Select the product name under Products to begin defining tests for the product as shown in Figure 23.

Dashboard Vendor: Sample Vendor

Sample Vendor (ID: ID 1) + Add Product Edit Vendor

<http://www.samplevendor.com>
 1287 enterprise way, DC, 20113
 John Doe (Manager)
 johndoe@samplevendor.com
 (111) 111-1111

2 Products

EH Product	C1		C2	C3			C4	
	Sample	QRDA-I	QRDA-III	Sample	QRDA-I	QRDA-III	QRDA-I	QRDA-III
✓ 0 Passing Tests								
✗ 0 Failing Tests								
○ 28 Not started Tests	3	3	3	3	3	3	5	5

Sample Product	C1		C2	C3			C4	
	Sample	QRDA-I	QRDA-III	Sample	QRDA-I	QRDA-III	QRDA-I	QRDA-III
✓ 0 Passing Tests								
✗ 0 Failing Tests								
○ 90 Not started Tests	4	18	18	4	18	18	5	5

Figure 23. Dashboard Displaying a Vendor with Two Products Added

3.4 Test Execution

Background

This process evaluates the capability of the health IT system under test (SUT) to electronically generate the proper eCQM artifacts for the eCQMs being certified.

The Test Proctor provides the Cypress v4.0 Test Data for the clinical quality measures for which the technology will be tested in the format selected by the EHR vendor.

Depending on the test, the vendor manually inputs or electronically downloads the patient test data from Cypress that is used to test their technology.

- Selecting C1 certification along with C2, C3, and C4 will provide the vendor with the following certification test options that allow a Test Proctor to examine the eCQMs implemented in their technology:
 - C1-C3 Record Sample tests, which will have only four predetermined measures for testing of C1 and C3 certifications. This tab validates the technology for C1 and C3 certifications by entering specified patient data for four measures. Certifiers will download a QRDA zip file of patients, which is uploaded into their technology and re-uploaded into Cypress.
 - C1-C3 (QRDA-I), which will contain measures (based on your selection of all eCQMs or Custom for either hospitals or professionals). This tab will test the technology's ability to record and export (C1) and submit (C3) measure-based data.
 - C2-C3 (QRDA-III), which tests the technology's ability to import and calculate (C2) and submit (C3) measure-based data. Certifiers will submit XML patient files exported from their technology to verify calculation and submission of reporting.

- C4 (QRDA-I and QRDA-III), which test the technology’s ability to filter patient records.

This process enables you to test the product based on the Certification Types and Measures Options you selected when you created the product.

3.4.1 Automated Measure Test Execution

C1 as well as a C2, C3, or C4 certification type all require automated measure test execution. Figure 24 shows C1 and C2 certification types selected for all hospital eCQMs with randomized and duplicate records to be included in the test data files created by Cypress. Products certifying to C2 criteria in addition to C1 will create a product that has a limited number of C1 record sample test measures, automated C1 measure test, and any other certification tests created.

Dashboard > Vendor: Sample Vendor > Add Product

Add Product

Name
Sample Product

Version

Description

Certification Types

- C1 Test
- C2 Test
- C3 Test
- C4 Test

Select the certification type Cypress should use to certify this product

Records Options

- Randomize Records
- Duplicate Records

Recommended for most robust testing.

Annual Update Bundle
Cypress bundle for the 2019 Reporting/Performance period (eCQM value sets as of May 4, 2018)

- Shift Records

Selecting Shift Records will move patient data forward into the appropriate reporting period. Otherwise patient data will remain in a previously completed calendar year.

Measures Options

- Eligible Hospital eCQMs
- Eligible Professional eCQMs
- All eCQMs
- Custom...

Indicate the clinical quality measures Cypress should use to certify this product. Testing will be performed on a measure-by-measure basis. Click 'Custom' to specify individual measures.

Add Product Cancel

Figure 24. C1-C2 Automated Entry Certification

Figure 25 shows the result of adding the C1-C2 certification.

Dashboard Vendor: Sample Vendor

'Sample Product' was created.

Sample Vendor (ID: ID 1) + Add Product Edit Vendor

<http://www.samplevendor.com>
 1287 enterprise way, DC, 20113
 John Doe (Manager)
 johndoe@samplevendor.com
 (111) 111-1111

2 Products

Sample Product	C1		C2	C3			C4	
	Sample	QRDA-I	QRDA-III	Sample	QRDA-I	QRDA-III	QRDA-I	QRDA-III
✓ 0 Passing Tests ✗ 0 Failing Tests ○ 36 Not started Tests	4	16	16					

Figure 25. Add Product for Automated Entry of Measure Data

To select a measure for testing, click on the product name shown in Figure 26.

Dashboard Vendor: Sample Vendor

'Sample Product' was created.

Sample Vendor (ID: ID 1) + Add Product Edit Vendor

<http://www.samplevendor.com>
 1287 enterprise way, DC, 20113
 John Doe (Manager)
 johndoe@samplevendor.com
 (111) 111-1111

2 Products

Sample Product	C1		C2	C3			C4	
Sample	QRDA-I	QRDA-III	Sample	QRDA-I	QRDA-III	QRDA-I	QRDA-III	
✓ 0 Passing Tests ✗ 0 Failing Tests ○ 36 Not started Tests	4	16	16					

Figure 26. Selecting A Product to Test

Figure 27 shows the certification tests created for C1-C2 Hospital measures. Note the tab for record sample that contains only four measures as well as tabs for C1 all Hospital and C2 certifications. The first Record Sample Test validates the technology for C1 certification by entering specified patient data for those identified measures. The second tab, C1 (QRDA-I), tests the technology's ability to record and export (C1), while the third tab, C2 (QRDA-III) tests the technology's ability to import and calculate (C2). Two sections appear, side by side, toward the top of the page: Product Status and Download Full Test Deck. On the left side of the page is the Product Status section that provides, for each Certification Type (based on the Measures Options you selected), a quick summary of the test cases that have passed, failed, and not yet started. On

the right side of the page is a section entitled Download Full Test Deck. This download contains a folder for each measure selected for this product. These folders contain XML documents for each patient associated with that measure.

Dashboard Vendor: Sample Vendor Product: Sample Product

Sample Product [Edit Product](#) [Download Report](#)

	C1		C2		C3		C4	
	Sample	QRDA-I	QRDA-III	Sample	QRDA-I	QRDA-III	QRDA-I	QRDA-III
✓ 0 Passing Tests								
✗ 0 Failing Tests								
○ 36 Not started Tests	4	16	16					

Download Full Test Deck

This download contains a folder for each measure selected for this product. Inside these folders are XML documents for each patient associated with that measure.

[Download All Patients \(.zip\)](#)

C1 Sample C1 (QRDA-I) C2 (QRDA-III)

Validate the EHR system for C1 certification by entering specified patient data for the following measures.

[View Record Sample](#)

Upload Results	C1 Upload Results	Status
○ Not Started	○ Not Started	○ Not Started

Data Criteria Verification	Status
CMS31v6 Hearing Screening Prior To Hospital Discharge	Not Started
CMS104v6 Discharged on Antithrombotic Therapy	Not Started
CMS105v6 Discharged on Statin Medication	Not Started
CMS107v6 Stroke Education	Not Started

Figure 27. Showing C1 Record Sample, C1 Automated, and C2 Product Measures

To execute a Test for C1 (QRDA-1), select that tab and select the desired measure to begin testing, using either the Upload Link (if you already have your zip file ready for upload), or click on the Measure Name to download a test file to upload for C1 Certification testing as shown in Figure 28. The upload button will display a file selection dialogue box to select your file. The Measure Name Link will take you to the screen shown in Figure 29.

CMS ID	Measure Name	C1 Results	Quick Upload	Last Updated
CMS108v6	Venous Thromboembolism Prophylaxis	○ Not Started	upload	○ 3 minutes ago
CMS190v6	Intensive Care Unit Venous Thromboembolism Prophylaxis	○ Not Started	upload	○ 3 minutes ago
CMS105v6	Discharged on Statin Medication	○ Not Started	upload	○ 3 minutes ago
CMS107v6	Stroke Education	○ Not Started	upload	○ 3 minutes ago
CMS102v6	Assessed for Rehabilitation	○ Not Started	upload	○ 3 minutes ago
CMS104v6	Discharged on Antithrombotic Therapy	○ Not Started	upload	○ 3 minutes ago

Figure 28. Product Measure Upload or Measure Name Selection

Once you have selected the Measure Name you want to test, Cypress displays the test page for that individual measure (e.g., CMS108v6) as shown in Figure 29.

Figure 29. Individual Measure Test Page

- Patient test data for the selected eCQMs of the specified test must be downloaded in the format required for the test.
- Click the **Download QRDA Category I (.zip)** button to download the test data for that selected eCQM. The downloaded zip file will contain duplicate and randomized patient records that your technology should correct for the uploaded portion of the test. The downloaded patient record test data will be contained in a zip file. Figure 30 shows an example filename entry.



Figure 30. Zip File of Patient Test Data for Selected eCQM

- If you click the **View Patients** link (shown in Figure 29), you will see a listing of the patients for that specific measure.
- Click **Get Known Good Results** link to download a zip file of patients that will pass the measure test you are planning to conduct as shown in Figure 31.

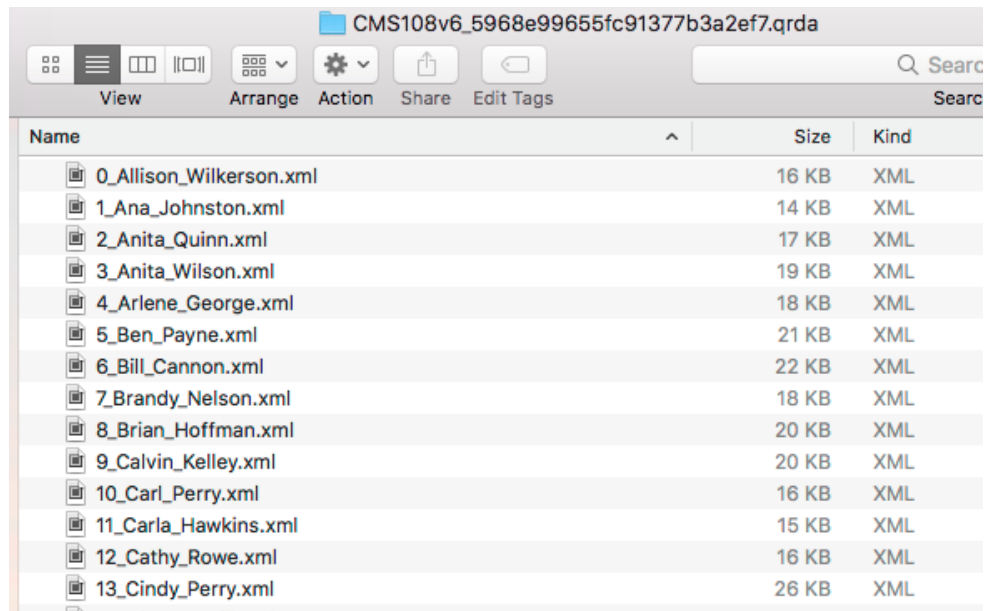


Figure 31. Listing of Zip File of XML Patient Test Data for Testing Selected eQCM

- Select a single patient record and open the XML from the zip file listing to view the information. Figure 32 presents an example screenshot.

```

CMS117v4_5717f0d667c28f4ffe43875a.debug Reporting period changed mood and class code/xml
<?xml version="1.0" encoding="utf-8"?>
<ClinicalDocument xmlns:xsi="http://www.w3.org/2001/XMLSchema-instance"
  xmlns="urn:h17-org:v3"
  xmlns:cda="urn:h17-org:v3">
  <!--
  *****
  CDA Header
  *****
  -->
  <realmCode code="US"/>
  <typeId root="2.16.840.1.113883.1.3" extension="POCD_HD000040"/>
  <!-- QRDA Category III Release 1 template ID (this template ID differs from QRDA III comment only
  template ID). -->
  <templateId root="2.16.840.1.113883.10.20.27.1.1"/>
  <id root='23440020-ff41-0133-b3b7-00505601057e' extension="CypressExtension"/>

  <!-- SHALL QRDA III document type code -->
  <code code="55184-6" codeSystem="2.16.840.1.113883.6.1" codeSystemName="LOINC"
    displayName="Quality Reporting Document Architecture Calculated Summary Report"/>
  <!-- SHALL Title, SHOULD have this content -->
  <title>QRDA Calculated Summary Report</title>
  <!-- SHALL -->
  <effectiveTime value="20160518161144"/>
  <confidentialityCode codeSystem="2.16.840.1.113883.5.25" code="N"/>
  <languageCode code="en"/>
  <!-- SHOULD The version of the file being submitted. -->
  <versionNumber value="1"/>
  <!-- SHALL contain recordTarget and ID - but ID is nulled to NA. This is an aggregate summary report.
  Therefore CDA's required patient identifier is nulled. -->
  <recordTarget>
    <patientRole>
      <id nullFlavor="NA"/>
    </patientRole>
  </recordTarget>

  <!-- SHALL have 1..* author. MAY be device or person.
  The author of the CDA document in this example is a device at a data submission vendor/registry. -->
  <author>
    <time value="20160518161144"/>
    <assignedAuthor>

```

Figure 32. Patient XML File for C2 Test

- Once the technology has generated the test results in the QRDA Category I format, the results are uploaded from that individual measure's test page under the Upload files section. For C2 and C3 testing, this upload would occur in QRDA Category III format.
- Click on **Select file** as shown in Figure 33, browse to the QRDA Category I file you want to upload, and click **Choose**.

Measure Test Information

Measure: Venous Thromboembolism Prophylaxis
 HQMF ID: 40280382-5ABD-FA46-015B-1F6B95092A9D
 CMS ID: CMS108v6

Provider Name: Graves, Danielle
 Provider NPI: 1513804843
 Provider TIN: 268221413
 Provider CCN: 242520

[View Patients](#)
[Get Known Good Result](#)

C1

QRDA Errors --
 Reporting Errors --
 Execution Date --

C2

QRDA Errors --
 Reporting Errors --
 Execution Date --

start

1 ⚡ Download Test Deck

Download and import this data into your EHR clinical quality measure calculator.

Download QRDA Category I (.zip)

2 ⚡ Upload Files

Upload results from the EHR system in the form of a zip file of QRDA Category I documents to get test results. This will automatically run a test execution.

Select file

Figure 33. Upload Test Execution Results

- The Test Proctor will then validate that the proper eCQM artifacts in QRDA Category I file format for the test being performed are electronically generated by the health IT SUT.
- Validation results will then be displayed in the Dashboard for that specific vendor's product as shown in Figure 34.

2 Products

EH Product	C1		C2	C3			C4	
	Sample	QRDA-I	QRDA-III	Sample	QRDA-I	QRDA-III	QRDA-I	QRDA-III
✓ 2 Passing Tests		1			1			
✗ 0 Failing Tests								
○ 26 Not started Tests	3	2	3	3	2	3	5	5

Sample Product	C1		C2	C3			C4	
	Sample	QRDA-I	QRDA-III	Sample	QRDA-I	QRDA-III	QRDA-I	QRDA-III
✓ 0 Passing Tests								
✗ 1 Failing Tests		1						
○ 35 Not started Tests	4	15	16					

Figure 34. Example of Test Execution Summary Results

3.4.2 Record Sample Test

To begin record sample testing (and validate the technology for C1 certification by entering specified patient data for specific measures), select the Record Sample Test tab and then select **View Test** as shown in Figure 35.

C1 + C3 Sample C1 + C3 (QRDA-I) C2 + C3 (QRDA-III) C4 (QRDA-I and QRDA-III)

Validate the EHR system for C1 and C3 certifications by entering specified patient data for the following measures.

[View Record Sample](#)

Upload Results	C1 Upload Results	C3 Upload Results	Status
<input type="radio"/> Not Started	<input type="radio"/> Not Started	<input type="radio"/> Not Started	<input type="radio"/> Not Started

Data Criteria Verification	Status
CMS32v7 Median Time from ED Arrival to ED Departure for Discharged ED Patients	Not Started
CMS55v6 Median Time from ED Arrival to ED Departure for Admitted ED Patients	Not Started
CMS11v6 Median Admit Decision Time to ED Departure Time for Admitted Patients	Not Started

Figure 35. Record Sample Test, Select "View Test"

As shown in Figure 36, this action will bring you to the Record Sample Checklist test page, which displays the status of each test on the right margin (i.e., Not Started, Passing, or Failing). The Record Sample Checklist page also displays a summary of each test and allows the user to check off (and save) a test when it has been completed.

[View Results](#)

Upload Results	C1 Upload Results	Status
<input type="radio"/> Not Started	<input type="radio"/> Not Started	<input type="radio"/> Not Started

Data Criteria Verification	Status
CMS32v8 Median Time from ED Arrival to ED Departure for Discharged ED Patients	Not Started

[Edit Test](#)

CMS32v8 Median Time from ED Arrival to ED Departure for Discharged ED Patients

Validated in QRDA	Data Criteria	Section	Required Attributes	Value Set(s)	Recorded Code/Attribute Value
	Encounter, Performed	Valuesets		Encounter Inpatient 2.16.840.1.113883.3.666.5.307 Emergency Department Visit 2.16.840.1.113883.3.117.1.7.1.292	Code <input type="text"/>
	Encounter, Order	Valuesets		Observation Services 2.16.840.1.113762.1.4.1111.143	Code <input type="text"/>

Figure 36. Record Sample Page

When choosing a code to demonstrate entry of a Record Sample data criteria, click on the allowable value sets to view a listing of valid codes as shown in Figure 37. Clicking on the allowable value sets will open a window displaying all the codes in the value sets as shown in Figure 38. The list is searchable, allowing a user to find an appropriate code for entry.

Validated in QRDA	Data Criteria	Section	Required Attributes	Value Set(s)	Recorded Code/Attribute Value
	Encounter, Performed	Valuesets		Encounter Inpatient 2.16.840.1.113883.3.666.5.307 Emergency Department Visit 2.16.840.1.113883.3.117.1.7.1.292	Code
	Encounter, Order	Valuesets		Observation Services 2.16.840.1.113762.1.4.1111.143	Code

Save

Figure 37. View listing of valid codes

Not Started

Data Criteria Verification

CMS32v8 Median Time from ED Arr

Edit Test

CMS32v8 Median Time from E

Validated in QRDA

Data Criteria

Encounter, Performed

Valuesets

Encounter, Order

Valuesets

Attributes

Attributes

Save

Status

Failing

Attribute Value

List of codes

Filter codes

Emergency hospital admission (procedure): 183452005

Hospital admission (procedure): 32485007

Hospital admission, elective (procedure): 8715000

Emergency department patient visit (procedure): 4525004

Close

2.16.840.1.113883.3.666.5.307 ✓ Code

Emergency Department Visit 4525004

2.16.840.1.113883.3.117.1.7.1.292

Attributes

2.16.840.1.113762.1.4.1111.143 ✓ Code

Observation Services 448851000124103

Attributes

Figure 38. Search for valid codes

Completing and saving a test, as shown in Figure 39, will then refresh the page and provide an updated status description for that specific test.

Validated in QRDA	Data Criteria	Section	Required Attributes	Value Set(s)	Recorded Code/Attribute Value
	Encounter, Performed	Valuesets		Encounter Inpatient 2.16.840.1.113883.3.666.5.307 Emergency Department Visit 2.16.840.1.113883.3.117.1.7.1.292	Code
	Encounter, Order	Valuesets		Observation Services 2.16.840.1.113762.1.4.1111.143	Code
		Attributes			
		Attributes			

Save

Figure 39. Complete and Save a Test

When all of your manual test measure entries are correct and have a completed checkmark, the select button will be enabled to allow upload of your XML files (zipped into a single file) into Cypress for certification as shown in Figure 40.

1 Record Sample Instructions

- Fill in the Data Criteria fields below.
 - If a Data Criteria has value sets listed, an appropriate code needs to be entered into the "Recorded Code" text box.
 - If an Attribute has a value set, an appropriate code needs to be entered into the "Recorded Attribute Code" text box.
 - Codes are validated upon saving.
 - Result, Date Times, and Related To are to be recorded as free text. ATLS will record the values they have observed being entered into the system under test.
- Create (at least) one patient for each measure below. Patients may be created using a user interface, or may be created as a structured document to be imported into the system under test.
 - There are no requirements on what format the structured data artifact must be. Could be CCDA, QRDA, or other formats.
 - This structured data artifact needs to be created at the time of certification
 - The created patients must contain all required Data Criteria, for the selected measures, to pass certification.
 - Export the created patients as QRDA Category I, and create a zip file.
- Upload zip file with created test patients.

2 Upload Files

Fill in the Data Criteria fields before you upload results from your EHR system.

Figure 40. Select File to Upload

3.4.3 CQM Filtering Test

The filter functionality included in this criterion allows a provider to query for eCQM results using one or a combination of data captured by the certified health IT for quality improvement and quality reporting purposes. It can also help identify health disparities, enable care quality improvement, and support providers in delivering more effective care to their patient populations. This certification criterion requires that a Health IT Module be capable of recording data (according to specified standards, where applicable) and filtering eCQM results at both patient and aggregate levels. These filters include, but are not limited to, practice site address, patient age, patient sex, and patient problem list.

- To begin eCQM filtering testing, click the C4 (QRDA-I and QRDA-III) Filtering Test tab, and click **start** on the Category I or Category III filtering criteria you are interested in testing, as shown in Figure 41.

C1 + C3 Sample C1 + C3 (QRDA-I) C2 + C3 (QRDA-III) **C4 (QRDA-I and QRDA-III)**

Test the EHR system's ability to filter patient records.

Filtering Criteria	QRDA Category I	QRDA Category III	Last Updated
Age/Ethnicities	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> an hour ago
NPI & TIN	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> an hour ago
NPI, TIN & Provider Location	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> an hour ago
Payers/Ethnicities	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> an hour ago
Races/Genders	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> start <input type="radio"/> upload	<input type="radio"/> an hour ago

Figure 41. Select a Category I or Category III to Test

- In this example, the Category I test page for Median Time from ED Arrival to ED Departure for Discharged ED Patients will be displayed as shown in Figure 42.

C1 | C2 | C3 | **C4**

Previous Test: CMS32v7 Next Test: CMS32v7

Filtering Test Information	QRDA Category I	QRDA Category III
Measure: Median Time from ED Arrival to ED Departure for Discharged ED Patients HQMF ID: 40280382-5A66-EAB9-015A-AF5BA5D72C52 CMS ID: CMS32v7 View Patients Get Known Good Result	QRDA Errors -- Reporting Errors -- Submission Errors -- Warnings -- Execution Date --	QRDA Errors -- Reporting Errors -- Submission Errors -- Warnings -- Execution Date -- start

1 Download Test Deck	2 Filter Patients	3 Upload Files
Download and import this data into your EHR clinical quality measure calculator. Download QRDA Category I (.zip)	Remove any patients not meeting the following criteria. Age As Of July 14, 2017 Minimum 62 Ethnicities Not Hispanic or Latino (code: 2186-5)	Upload results from the EHR system in the form of a zip file of QRDA Category I documents to get test results. This will automatically run a test execution. <input type="text"/> Select file

Figure 42. Category I Test Page for Median Time from ED Arrival to ED Departure for Discharged ED Patients

- Patient test data for the specified test must be downloaded in the format required for the test. This step, and those following, adhere to the same process as the steps outlined in the *Measure Tests* section, and will not be repeated here.

3.5 Test Execution Success Criteria

The criteria to determine a successful test outcome depend on whether the health IT product is being certified against the EP eCQMs or the EH eCQMs. The criteria for test execution success are as follows:

- For EP eCQMs**, a successful test outcome is one in which the following conditions are true:

1. There were no XML validation errors in either the QRDA Category I submitted data or the QRDA Category III submitted data.
 2. All of the eCQM results calculated and submitted by the health IT SUT exactly match the values that Cypress v4.0 was expecting.
- **For EH eCQMs**, a successful test outcome is one in which the following conditions are true:
 1. There were no XML validation errors in either the QRDA Category I submitted data or the QRDA Category III submitted data.
 2. All of the eCQM results calculated and submitted by the health IT SUT for discrete measures exactly match the values that Cypress v4.0 was expecting.
 3. The eCQM results calculated and submitted by the health IT SUT for continuous variable tests are within a defined delta of the value that Cypress v4.0 was expecting.

For both types of technologies, it is acceptable to have XML validation *warnings* generated by the Cypress validation process. These warnings do not constitute a test failure; however, the Test Proctor should review the warnings generated and record any relevant observations about the reasons for the warnings.

Cypress groups failed test cases into three categories: (1) QRDA errors associated with logic and improper use of the QRDA standard, (2) reporting errors associated with errors in the calculation and aggregation of measure data for reporting purposes, and (3) submission errors associated with improper logic and formatting for submitting measure data to CMS. In addition to errors, Cypress will flag and report on warnings that indicate non-conformance with the CMS Implementation Guide (and associated schematron validation). Note, for health IT products not certifying for reporting (C3), non-conformance with the HL7 QRDA Implementation Guide will be treated as warnings. Figure 42 provides an example of measure test failure results.

The screenshot displays the Cypress workflow interface for a Measure Test. At the top, there are navigation buttons for 'Previous Test: CMS107v6' and 'Next Test: CMS111v6'. The main content is divided into two columns, C1 and C2. Column C1 shows 'Measure Test Information' for 'Venous Thromboembolism Prophylaxis' with various IDs and provider details. It also shows 'QRDA Errors: 0', 'Reporting Errors: 10', and 'Execution Date: July 14, 2017 4:28pm'. A status indicator shows 'Failing'. Column C2 shows 'QRDA Errors: --', 'Reporting Errors: --', and 'Execution Date: --', with a 'start' button. Below this are two main actions: 'Download Test Deck' and 'Upload Files'. The 'Results' section is highlighted in red and shows 'Failed with 10 errors'. It lists 'Missing or Duplicate Files' (61 files expected but was 67) and 'Errors and Warnings' for three XML files: '17_Dale_Parker.xml' (1 error), '27_Ella_Guzman.xml' (1 error), and '55_Sally_Reeves.xml' (7 errors). A specific error message is shown: 'Patient 'DALE PARKER' not expected to be returned.'

Figure 43. Measure Test Failure Messages

3.6 Submit

Electronically Submit Generated eCOM Artifacts

This functionality allows evaluation of the capability to electronically submit (a) calculated quality measures in accordance with the standard and implementation specifications, and (b) exported patient data sufficient to allow external calculation as follows:

- The Test Proctor commands the health IT SUT to generate and electronically submit the patient-level export in the QRDA Category I format for the clinical quality measures being tested.
- The Test Proctor commands the health IT SUT to generate and electronically submit an aggregate report in the QRDA Category III format of the clinical quality measures calculated in the test.

- The Test Proctor validates that the calculated clinical quality measures are submitted in accordance with the QRDA Category III standard and implementation specifications by uploading the QRDA Category III XML via the Cypress v4.0 User Interface and the Cypress-supplied XML Schema validation.
- The Test Proctor validates that the exported patient-level eCQM data are submitted in accordance with the QRDA Category I standard and implementation specifications by uploading the QRDA Category I XML via the Cypress v4.0 User Interface and the Cypress-supplied XML Schema validation.

3.7 Verify

Verify Electronic and Accurate Generation of Clinical Quality Measure Artifacts

This functionality allows evaluation of the capability to electronically and accurately generate eCQM artifacts appropriate for each phase of the test procedure as follows:

- After the Test Proctor validates the submission of the QRDA Category III, the Test Proctor evaluates and displays the accuracy of the submitted clinical quality measure results via the Cypress v4.0 User Interface.
- The Test Proctor generates a test artifact bundle containing all test data used for this test execution, all products generated and submitted by the health IT SUT, and any other additional notes or information that the Test Proctor deems relevant into a single archive file that is cryptographically signed.

Acronyms

Acronym	Definition
----------------	-------------------

ACO	Accountable Care Organization
------------	-------------------------------

ATL	Authorized Testing Lab
------------	------------------------

CAMH	CMS Alliance to Modernize Healthcare
-------------	--------------------------------------

CMS	Centers for Medicare & Medicaid Services
------------	--

CQM	Clinical Quality Measure
------------	--------------------------

eCQM	Electronic Clinical Quality Measure
-------------	-------------------------------------

EH	Eligible Hospital
-----------	-------------------

EHR	Electronic Health Record
------------	--------------------------

EP	Eligible Professional
-----------	-----------------------

FFRDC	Federally Funded Research and Development Center
--------------	--

HHS	Department of Health and Human Services
------------	---

HL7	Health Level Seven International
------------	----------------------------------

HTML	Hypertext Markup Language
-------------	---------------------------

IG	Implementation Guide
-----------	----------------------

IT	Information Technology
-----------	------------------------

NIST	National Institute of Standards and Technology
-------------	--

ONC	Office of the National Coordinator for Health Information Technology
------------	--

QDM	Quality Data Model
------------	--------------------

QRDA	Quality Reporting Document Architecture
-------------	---

SUT	System Under Test
------------	-------------------

XML	Extensible Markup Language
------------	----------------------------